

External Hex Implant System

Product Catalog



Important Product Information

Biomet 3i Dental Implants

For detailed product information on all Biomet 3i Dental Implants, refer to the Biomet 3i Dental Implant IFU (P-IIS086GI) located at ifu.biomet3i.com.

Biomet 3i Restorative Products

For detailed product information on all Biomet 3i Restorative Products, refer to the Biomet 3i Restorative Products IFU (P-IIS086GR) located at ifu.biomet3i.com.

Table of Contents

Implants

Tapered and Parallel Walled External Hex Implants	4
T3® Tapered Implants With DCD® Surface	4
T3 Parallel Walled Implants With DCD Surface	4
T3 Tapered	4
T3 Parallel Walled	4

Site Preparation Technologies

Surgical Kits	5
Tapered Implant Surgical Kits	5
Parallel Walled Surgical Kits	8
Surgical Drills	10
W & H Surgical Drilling Unit And Osstell ISQ Module	10
Advanced Cutting Technology® (ACT®) Twist Drills	11
Quad Shaping Drills For Tapered Implants	11
Miscellaneous Drills	11
Surgical Components	12
Dense Bone Taps For Parallel Walled Implants	12
Dense Bone Taps For Tapered Implants	12
Tapered Implant Depth Indicators	13
Direction Indicators	13
Implant Mounts	13
Bone Profilers for External Hex Connection	14
Bone Profilers for External Hex Connection Low Profile	14
Tapered Osteotomes	14
Summers Osteotomes	15
Sinus Elevation	15
Trepine Burs	15
Miscellaneous Instrumentation	16

Restorative Components


Healing Abutments	19
BellaTek® Encode®	19
EP® One-piece	19
Provisional Restorations	20
PreFormance® Posts	20
Temporary Cylinders	20
Definitive Restorations	21
GingiHue® Posts	21

UCLA Abutments	21
GingiHue Post And UCLA Abutment Components	22
Low Profile Abutments	23
Low Profile Abutment Components	23
Overdenture Restorations	24
LOCATOR R-Tx® Abutments	24
LOCATOR® Abutments	25
Screws	26
Abutment Screws	26
Retaining Screws	26
Waxing Screws And Try-In Screws	26
BellaTek Bars and Frameworks	27
Mechanical Driver Kits	28
Prosthodontic Screwdriver	29
Drivers and Driver Tips	30
Miscellaneous Restorative Products	31
Regenerative Product Portfolio	32

Implants


T3 Tapered Implants With DCD Surface

Commercially Pure Titanium

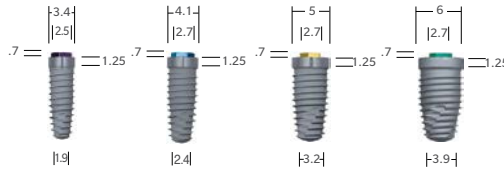

T3 Parallel Walled Implants With DCD Surface

Commercially Pure Titanium

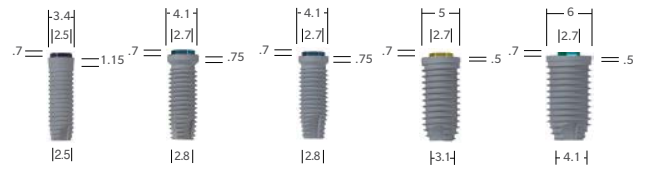

Length	3.25 mmD	4.0 mmD	5.0 mmD	6.0 mmD
6.5 mm	—	—	—	—
8.5 mm	BNET3285	BNET485	BNET585	BNET685
10 mm	BNET3210	BNET410	BNET510	BNET610
11.5 mm	BNET3211	BNET411	BNET511	BNET611
13 mm	BNET3213	BNET413	BNET513	BNET613
15 mm	BNET3215	BNET415	BNET515	BNET615
18 mm	—	—	—	—

3.25 mmD	3.75 mmD	4.0 mmD	5.0 mmD	6.0 mmD
BNES365	BNES3765	BNES465	BNES565	BNES665
BNES385	BNES3785	BNES485	BNES585	BNES685
BNES310	BNES3710	BNES410	BNES510	BNES610
BNES311	BNES3711	BNES411	BNES511	BNES611
BNES313	BNES3713	BNES413	BNES513	BNES613
BNES315	BNES3715	BNES415	BNES515	BNES615
BNES318	BNES3718	BNES418	BNES518	BNES618

T3 Tapered Implants

Commercially Pure Titanium

Length	3.25 mmD	4.0 mmD	5.0 mmD	6.0 mmD
6.5 mm	—	—	—	—
8.5 mm	BOET3285	BOET485	BOET585	BOET685
10 mm	BOET3210	BOET410	BOET510	BOET610
11.5 mm	BOET3211	BOET411	BOET511	BOET611
13 mm	BOET3213	BOET413	BOET513	BOET613
15 mm	BOET3215	BOET415	BOET515	BOET615
18 mm	—	—	—	—

T3 Parallel Walled Implants

Commercially Pure Titanium

3.25 mmD	3.75 mmD	4.0 mmD	5.0 mmD	6.0 mmD
BOES365	BOES3765	BOES465	BOES565	BOES665
BOES385	BOES3785	BOES485	BOES585	BOES685
BOES310	BOES3710	BOES410	BOES510	BOES610
BOES311	BOES3711	BOES411	BOES511	BOES611
BOES313	BOES3713	BOES413	BOES513	BOES613
BOES315	BOES3715	BOES415	BOES515	BOES615
BOES318	BOES3718	BOES418	BOES518	BOES618

Cover Screw 1.0 mmH (included)	MMCS1	CS375	CS500	CS600
Cover Screw Headless	CS275	CS275	CS275	CS275

MMCS1	CS375	CS375	CS500	CS600
CS275	CS275	CS275	CS275	CS275

Tapered Implant Surgical Kits

QNTSK40 Premium Kit



SLIMKTE Slim Kit - Certain And External Hex



Description	Item No.	Premium Kit	Upgrade Kit	Starter (Basic) Kit	Certain/External Hex
		QNTSK40	QNTSK40U	QNTSK20	SLIMKTE
Quad Shaping Drill, 3.25 mmD x 8.5 mmL	QSD3285	•	•		•
Quad Shaping Drill, 3.25 mmD x 10 mmL	QSD3210	•	•	•	•
Quad Shaping Drill, 3.25 mmD x 11.5 mmL	QSD3211	•	•	•	•
Quad Shaping Drill, 3.25 mmD x 13 mmL	QSD3213	•	•	•	•
Quad Shaping Drill, 3.25 mmD x 15 mmL	QSD3215	•	•		
Quad Shaping Drill, 4 mmD x 8.5 mmL	QSD485	•	•		•
Quad Shaping Drill, 4 mmD x 10 mmL	QSD410	•	•	•	•
Quad Shaping Drill, 4 mmD x 11.5 mmL	QSD411	•	•	•	•
Quad Shaping Drill, 4 mmD x 13 mmL	QSD413	•	•	•	•
Quad Shaping Drill, 4 mmD x 15 mmL	QSD415	•	•		
Quad Shaping Drill, 5 mmD x 8.5 mmL	QSD585	•	•		
Quad Shaping Drill, 5 mmD x 10 mmL	QSD510	•	•	•	
Quad Shaping Drill, 5 mmD x 11.5 mmL	QSD511	•	•	•	
Quad Shaping Drill, 5 mmD x 13 mmL	QSD513	•	•	•	
Quad Shaping Drill, 5 mmD x 15 mmL	QSD515	•	•		
Quad Shaping Drill, 6 mmD x 8.5 mmL	QSD685	•	•		
Quad Shaping Drill, 6 mmD x 10 mmL	QSD610	•	•		
Quad Shaping Drill, 6 mmD x 11.5 mmL	QSD611	•	•		
Quad Shaping Drill, 6 mmD x 13 mmL	QSD613	•	•		
Quad Shaping Drill, 6 mmD x 15 mmL	QSD615	•	•		
Certain® Driver Replacement O-Rings (10-pack)	IRORDR	•	•	•	•
Internal Connection Universal Placement Driver Tip - Long	IIPDTUL	•			
Internal Connection Universal Placement Driver Tip - Short	IIPDTUS	•			•
Dense Bone Tap, 3.25 mmD x 8.5 mmL	NTAP3285	•	•		•
Dense Bone Tap, 3.25 mmD x 10 mmL	NTAP3210	•	•	•	•
Dense Bone Tap, 3.25 mmD x 11.5 mmL	NTAP3211	•	•	•	•
Dense Bone Tap, 3.25 mmD x 13 mmL	NTAP3213	•	•	•	•
Dense Bone Tap, 3.25 mmD x 15 mmL	NTAP3215	•	•		
Dense Bone Tap, 4 mmD x 8.5 mmL	NTAP485	•	•		•
Dense Bone Tap, 4 mmD x 10 mmL	NTAP410	•	•	•	•
Dense Bone Tap, 4 mmD x 11.5 mmL	NTAP411	•	•	•	•
Dense Bone Tap, 4 mmD x 13 mmL	NTAP413	•	•	•	•
Dense Bone Tap, 4 mmD x 15 mmL	NTAP415	•	•		

Surgical Kits

Site Preparation Technologies

Tapered Implant Surgical Kits (Continued)

Description	Item No.	Premium Kit	Upgrade Kit	Starter (Basic) Kit	Certain/External Hex
		QNTSK40	QNTSK40U	QNTSK20	SLIMKTE
Dense Bone Tap, 5 mmD x 8.5 mmL	NTAP585	•	•		
Dense Bone Tap, 5 mmD x 10 mmL	NTAP510	•	•	•	
Dense Bone Tap, 5 mmD x 11.5 mmL	NTAP511	•	•	•	
Dense Bone Tap, 5 mmD x 13 mmL	NTAP513	•	•	•	
Dense Bone Tap, 5 mmD x 15 mmL	NTAP515	•	•		
Dense Bone Tap, 6 mmD x 8.5 mmL	NTAP685	•	•		
Dense Bone Tap, 6 mmD x 10 mmL	NTAP610	•	•		
Dense Bone Tap, 6 mmD x 11.5 mmL	NTAP611	•	•		
Dense Bone Tap, 6 mmD x 13 mmL	NTAP613	•	•		
Dense Bone Tap, 6 mmD x 15 mmL	NTAP615	•	•		
Tapered Implant Dense Bone Tap Kit Tray	NTAPK	•	•	•	
Tapered Implant Depth Indicator, 3.25 mmD x 8.5 mmL 3ea.	NTDI3285*	•	•		•
Tapered Implant Depth Indicator, 3.25 mmD x 10 mmL	NTDI3210	•	•	•	•
Tapered Implant Depth Indicator, 3.25 mmD x 11.5 mmL	NTDI3211	•	•	•	•
Tapered Implant Depth Indicator, 3.25 mmD x 13 mmL	NTDI3213	•	•	•	•
Tapered Implant Depth Indicator, 3.25 mmD x 15 mmL	NTDI3215	•	•		
Tapered Implant Depth Indicator, 4 mmD x 8.5 mmL 3ea.	NTDI485*	•	•		•
Tapered Implant Depth Indicator, 4 mmD x 10 mmL	NTDI410	•	•	•	•
Tapered Implant Depth Indicator, 4 mmD x 11.5 mmL	NTDI411	•	•	•	•
Tapered Implant Depth Indicator, 4 mmD x 13 mmL	NTDI413	•	•	•	•
Tapered Implant Depth Indicator, 4 mmD x 15 mmL	NTDI415	•	•		
Tapered Implant Depth Indicator, 5 mmD x 8.5 mmL 3ea.	NTDI585	•	•		
Tapered Implant Depth Indicator, 5 mmD x 10 mmL	NTDI510	•	•	•	
Tapered Implant Depth Indicator, 5 mmD x 11.5 mmL	NTDI511	•	•	•	
Tapered Implant Depth Indicator, 5 mmD x 13 mmL	NTDI513	•	•	•	
Tapered Implant Depth Indicator, 5 mmD x 15 mmL	NTDI515	•	•		
Tapered Implant Depth Indicator, 6 mmD x 8.5 mmL 3ea.	NTDI685	•	•		
Tapered Implant Depth Indicator, 6 mmD x 10 mmL	NTDI610	•	•		
Tapered Implant Depth Indicator, 6 mmD x 11.5 mmL	NTDI611	•	•		
Tapered Implant Depth Indicator, 6 mmD x 13 mmL	NTDI613	•	•		
Tapered Implant Depth Indicator, 6 mmD x 15 mmL	NTDI615	•	•		
Certain Countersink Drill, 4 mmD	ICD100	•	•	•	•
Empty Surgical Tray	QNTSKT	•		•	
Open End Wrench	CW100	•		•	•
Ratchet Wrench	WR150	•		•	
High Torque Indicating Ratchet Wrench	H-TIRW**				•
Ratchet Extension (Short), 6 mmL	RE100	•		•	•
Ratchet Extension (Long), 15 mmL	RE200	•		•	

*One (1) each for SLIMKTE.

**H-TIRW, L-TIRW and associated adapters are manufactured by Elos Med Tech and distributed by Zimmer Biomet Dental - Packaged Individually.

Tapered Implant Surgical Kits (Continued)

Description	Item No.	Premium Kit	Upgrade Kit	Starter (Basic) Kit	Certain/External Hex
		QNTSK40	QNTSK40U	QNTSK20	SLIMKTE
Implant Depth Gauge, 20 mmL	DP020	•			
Narrow Posterior Hexed Driver, 17 mmL	PHD00N	•		•	•
Posterior Large Hexed Driver, 17 mmL	PHD02N	•		•	•
Narrow Right Angle Large Hexed Driver Tip, 24 mmL	RASH3N	•		•	
Direction Indicator, 2 mmD x 10 mmL 3ea.	DI100	•			
Handpiece Connector	MDR10	•			•
Implant Mount, 3.4 mmD x 15 mmL	MMC15	•			•
ACT Pointed Starter Drill	ACTPSD	•			•
ACT Reusable Twist Drill, 2 mmD x 10 mmL	ACT2010	•			
ACT Reusable Twist Drill, 2 mmD x 15 mmL	ACT2015	•			•
ACT Reusable Twist Drill, 2 mmD x 20 mmL	ACT2020	•		•	
ACT Drill Extension	ACTDE	•			•

Surgical Kits

Site Preparation Technologies

Parallel Walled Surgical Kits

For External Hex Connection Implants

Description	Item No.	Premium Kit	Standard Kit	Starter (Basic) Kit
		PSKT30	PSKT20	PSKT 10
Plastic Surgical Tray Organizer	PTT300I	•	•	•
Plastic Tray Organizer for PTT300I	PTT100	•	•	
ACT Reusable Twist Drill, 2 mmD x 10 mmL	ACT2010	•	•	
ACT Reusable Twist Drill, 2 mmD x 15 mmL	ACT2015	•	•	
ACT Reusable Twist Drill, 2 mmD x 20 mmL	ACT2020	•	•	
ACT Reusable Twist Drill, 2.75 mmD x 10 mmL	ACT2710	•	•	
ACT Reusable Twist Drill, 2.75 mmD x 15 mmL	ACT2715	•	•	
ACT Reusable Twist Drill, 2.75 mmD x 20 mmL	ACT2720	•	•	
ACT Reusable Twist Drill, 3.0 mmD x 10 mmL	ACT3010	•	•	
ACT Reusable Twist Drill, 3.0 mmD x 15 mmL	ACT3015	•	•	
ACT Reusable Twist Drill, 3.0 mmD x 20 mmL	ACT3020	•	•	
ACT Reusable Twist Drill, 3.25 mmD x 10 mmL	ACT3210	•	•	
ACT Reusable Twist Drill, 3.25 mmD x 15 mmL	ACT3215	•	•	
ACT Reusable Twist Drill, 3.25 mmD x 20 mmL	ACT3220	•	•	
ACT Reusable Twist Drill, 3.85 mmD x 20 mmL	ACT3820	•	•	
ACT Reusable Twist Drill, 4.25 mmD x 8.5 mmL	ACT4285	•		
ACT Reusable Twist Drill, 4.25 mmD x 13 mmL	ACT4213	•		
ACT Reusable Twist Drill, 4.25 mmD x 18 mmL	ACT4218	•		
ACT Reusable Twist Drill, 5.25 mmD x 8.5 mmL	ACT5285	•		
ACT Reusable Twist Drill, 5.25 mmD x 13 mmL	ACT5213	•		
ACT Reusable Twist Drill, 5.25 mmD x 18 mmL	ACT5218	•		
ACT Drill Extension	ACTDE	•	•	
Pilot Drill, 2-3.0 mmD	PD100	•	•	
Countersink Drill, 4.1 mmD	CD100	•	•	
Countersink Drill, Osseotite XP 4/5, Prevail 4/5/4	CD4500	•		
Countersink/Pilot Drill, 5 mmD	CD500	•		
Countersink Drill, Osseotite XP 5/6, Prevail 5/6/5	CD5600	•		
Countersink/Pilot Drill, 6 mmD	CD600	•		
Implant Dense Bone Tap, 3.25 mmD x 18 mmL	MTAP2	•	•	
Implant Dense Bone Tap, 4 mmD x 13 mmL	TAP413	•	•	
Implant Dense Bone Tap, 5 mmD x 13 mmL	TAP53S	•		
Implant Dense Bone Tap, 6 mmD x 13 mmL	TAP63S	•		
Osseotite® 2 Dense Bone Tap, 5 mmD x 7-13 mmL	XTAP53S	•		
Osseotite 2 Dense Bone Tap, 6 mmD x 7-13 mmL	XTAP63S	•		

Parallel Walled Surgical Kits (Continued)

Description	Item No.	Premium Kit	Standard Kit	Starter (Basic) Kit
		PSKT30	PSKT20	PSKT20
Narrow Small Hexed Hand Driver, 17 mmL	PHD00N	•	•	•
Narrow Large Hexed Hand Driver, 17 mmL	PHD02N	•	•	•
Narrow Large Hexed Driver, Tip 24 mmL	RASH3N	•	•	•
Handpiece Connector	MDR10	•	•	•
Open End Wrench	CW100	•	•	•
Ratchet Wrench	WR150	•	•	•
Ratchet Extension (Short), 6 mmL	RE100	•	•	•
Ratchet Extension (Long), 15 mmL	RE200	•	•	•
Implant Depth Gauge, 20 mmL	DP020	•	•	•
Implant Mount, 3.4 mmD x 15 mmL	MMC15	•	•	
Direction Indicator, 2 mmD x 10 mmL 3ea.	DI100	•	•	
Stainless Steel Round Drill, 2 mmD	RD100	•	•	

Surgical Drills

Site Preparation Technologies

W & H Surgical Drilling Unit And Osstell ISQ Module

The surgical drill system is ideal for implantology with its automatic thread cutter function, automatic torque control, and the Osstell ISQ module for measuring implants stability.



Description	Item No.
Drill Systems	
SI-1023 control unit, 230 V	30288000
SI-1015 control unit, 120 V	30289000
Motors	
EM-19 LC electric motor for SI-1015, w/LED & light contacts (LC), 1.8 m cable	30281000
EM-19 electric motor for SI-1015, without LED+ & light contacts (LC), 1.8 m cable	30185000
EM-19 LC electric motor for SI-1015, w/light contacts (LC), 3.5 m cable	30281001
Handpieces	
WS-75 L, contra-angle 20:1, mini LED+ for EM-19 LC motor	30033000
WS-56 L, contra-angle 1:1, mini LED+ for EM-19 LC motor	30040000
WS-56 L G, contra-angle 1:1, self-generating mini LED+	30039000
WS-75 L G, contra-angle 20:1, self-generating mini LED+	30032000
Foot Controls	
S-NW wireless foot control w/CAN dongle; compatible w/SI-1023, SI-1015	30264000
S-NW wireless foot control w/SPI dongle; compatible w/ SI-915 & Piezomed SA-320	30264001
S-N2 foot control w/cable, compatible w/SI-1015, SI-1023	30285000
Accessories	
W&H Osstell ISQ module, for SI-1015 ,SI-1023	30210000
W&H Osstell Measuring Probe	07721100
Wifi dongle CAN-Bus; SI-1015, SI-1023	07759700
Wifi dongle SPI; SI-915 & Piezomed SA-320	07795800
Universal Motor Holder	07721800
W&H Osstell Test Peg	07849900
SmartPeg Mount	07460300
SmartPegs	
W&H SmartPeg Type 1 - 100353, Pack of 5	08009800
W&H SmartPeg Type 4 - 100350, Pack of 5	08010120
W&H SmartPeg Type 15 - 100386, Pack of 5	08009860
W&H SmartPeg Type 26 - 100425, Pack of 5	08009970
W&H SmartPeg Type 27 - 100431, Pack of 5	08009980
W&H SmartPeg Type 30 - 100436, Pack of 5	08010010
W&H SmartPeg Type 32 - 100440, Pack of 5	08010020
W&H SmartPeg Type 33 - 100442, Pack of 5	08010030
W&H SmartPeg Type 34 - 100444, Pack of 5	08010040
W&H SmartPeg Type 35 - 100446, Pack of 5	08010050
W&H SmartPeg Type 45 - 100472, Pack of 5	08010150
W&H SmartPeg Type 60 - 100543, Pack of 5	08010620

Advanced Cutting Technology (ACT) Twist Drills

Features include:

- Two-flute design for efficient cutting
- Alternating lines and bands enhance depth mark visibility and drill orientation in the osteotomy
- Matte finish to reduce glare
- Non-Irrigated Reusable



Implant Lengths	Drill Lengths	2 mmD	2.3 mmD	2.75 mmD	3 mmD	3.15 mmD	3.25 mmD	3.85 mmD	4.25 mmD	4.85 mmD	5.25 mmD
7 – 8.5 mm	8.5 mm	—	—	—	—	—	—	—	ACT4285	ACT4885	ACT5285
7 – 10 mm	10 mm	ACT2010	—	ACT2710	ACT3010	ACT3110	ACT3210	ACT3810	—	—	—
7 – 13 mm	13 mm	—	—	—	—	—	—	—	ACT4213	ACT4813	ACT5213
7 – 15 mm	15 mm	ACT2015	—	ACT2715	ACT3015	ACT3115	ACT3215	ACT3815	—	—	—
7 – 18 mm	18 mm	—	—	—	—	—	—	—	ACT4218	ACT4818	ACT5218
7 – 20 mm	20 mm	ACT2020	—	ACT2720	ACT3020	ACT3120	ACT3220	ACT3820	—	—	—

Quad Shaping Drills For Tapered Implants

Features include:


- Quad Shaping Drills (QSDs) use stepped depth marks for accuracy in creating the osteotomy
- QSDs have end cutting ability
- QSDs are color-coded for platform recognition



Drill Lengths	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 mm	QSD3285	QSD485	QSD585	QSD685
10 mm	QSD3210	QSD410	QSD510	QSD610
11.5 mm	QSD3211	QSD411	QSD511	QSD611
13 mm	QSD3213	QSD413	QSD513	QSD613
15 mm	QSD3215	QSD415	QSD515	QSD615

Miscellaneous Drills

Description	Disposable	Reusable
Round Drill, 2 mm	DR100	RD100
ACT Pointed Starter Drill	—	ACTPSD
Pilot Drill, 2-3 mm	DP100	PD100
Countersink Drill - External Connection 4.1 mm	DC100	CD100
Countersink Drill, 4/5 mm	—	CD4500
Countersink/Pilot Drill, 5 mm	DC500	CD500
Countersink Drill, 5/6 mm	—	CD5600
Countersink/Pilot Drill, 6 mm	DC600	CD600

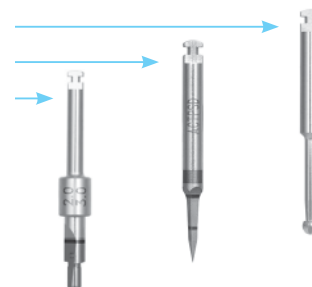

Surgical Components

Site Preparation Technologies

Dense Bone Taps For Parallel Walled Implants



Implant Lengths	3.25 mmD	3.75 mmD	4 mmD	5 mmD	6 mmD
7 – 8.5 mm	—	—	—	TAP58S	TAP68S
7 – 10 mm	—	TAP10	TAP410	—	—
7 – 13 mm	—	TAP13	TAP413	TAP53S	TAP63S
7 – 18 mm	—	—	—	TAP518S	TAP618S
7 – 20 mm	—	TAP20	TAP420	—	—
8.5 – 18 mm	MTAP1 (18 mL)	—	—	—	—
8.5 – 18 mm	MTAP2 (27 mL)	—	—	—	—

Dense Bone Taps For T3 Implants

6.5/7 – 8.5 mm (T3 Implants)	—	—	—	XTAP58S	XTAP68S
6.5/7 – 13 mm (T3 Implants)	—	—	—	XTAP53S	XTAP63S
6.5/7 – 18 mm (T3 Implants)	—	—	—	XTAP518S	XTAP618S

Dense Bone Taps For Tapered Implants



Implant Lengths	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 mm	NTAP3285	NTAP485	NTAP585	NTAP685
10 mm	NTAP3210	NTAP410	NTAP510	NTAP610
11.5 mm	NTAP3211	NTAP411	NTAP511	NTAP611
13 mm	NTAP3213	NTAP413	NTAP513	NTAP613
15 mm	NTAP3215	NTAP415	NTAP515	NTAP615

NTAPK

Dense Bone Tap Kit

NOTE: Kit includes all of the Dense Bone Taps listed above.



Tapered Implant Depth Indicators

Features include:

- Tapered Implant Depth Indicators (NTDIs) verify the position of the implant platform prior to placement
- NTDIs are color-coded for platform recognition




Implant Lengths	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 mm	NTDI3285	NTDI485	NTDI585	NTDI685
10 mm	NTDI3210	NTDI410	NTDI510	NTDI610
11.5 mm	NTDI3211	NTDI411	NTDI511	NTDI611
13 mm	NTDI3213	NTDI413	NTDI513	NTDI613
15 mm	NTDI3215	NTDI415	NTDI515	NTDI615

Also available in a kit:

NTDIK


Depth/Direction Indicator Kit

NOTE: Kit includes all of the indicators listed to the left.

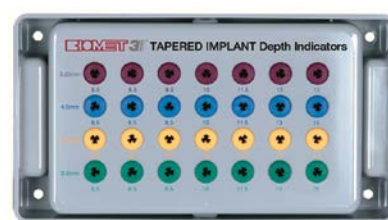


Direction Indicators

Description	Item No.
2 mm/3 mmD x 10 mmL	DI100
2 mm/3 mmD x 15 mmL	DI200
2.3 mm/3 mmD x 10 mmL, Anodized Blue	DI2310
2.3 mm/3 mmD x 15 mmL, Anodized Gold	DI2315

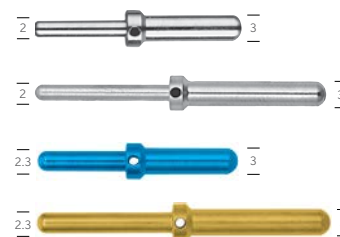

Implant Mounts

Description	Item No.
3.0 mmL Implant Mount	MMC03
15 mmL Implant Mount	MMC15
15 mmL Implant Carrier	IC015

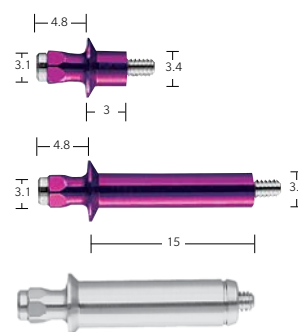

Surgical Components

Site Preparation Technologies

Handpiece Bone Profilers (Packaged With Guide Pin)

Description	Item No.
Bone Profiler, 3.4 mmD x 3.8 mmP	BP340
Bone Profiler, 3/4, 4.1 mmD x 5 mmP	BP450
Bone Profiler, 3/4, 4.1 mmD x 6 mmP	BP460
Bone Profiler, 3/4, 4.1 mmD x 7.5 mmP	BP475
Bone Profiler, 4/5, 5 mmD x 5 mmP	BP550
Bone Profiler, 4/5, 5 mmD x 6 mmP	BP560
Bone Profiler, 4/5, 5 mmD x 7.5 mmP	BP575
Bone Profiler, 5/6, 6 mmD x 6 mmP	BP660
Bone Profiler, 5/6, 6 mmD x 7.5 mmP	BP675



Low Profile Abutment Bone Profilers

Description	Item No.
Low Profile Abutment Bone Profiler, 3.4 mmD	LPCBP3
Low Profile Abutment Bone Profiler, 4.1 mmD	LPCBP4
Low Profile Abutment Bone Profiler, 5 mmD	LPCBP5



Bone Profiler Guide Pins

Description	Item No.
Bone Profiler Guide Pin, 4.1, 5 & 6 mmD	BPGUIDE

Bone Profiler Organizers And Kits

Description	Item No.
Bone Profiler Organizer Box, 4.1 mmD	BPKITB
Bone Profiler Organizer Box, 5 & 6 mmD	BPAKTB
Bone Profiler Organizer Kit	BB001
Bone Profiler Kit - For Use With 4.1 mmD Implants Contains: BP450, BP460, BP475, BB001	BPKIT
Bone Profiler Kit - For Use With 5 mmD or 6 mmD Implants Contains: BP550, BP560, BP575, BP660, BP675, BB001	BPAKT

Tapered Osteotomes

Available in straight and angled designs for use with Tapered Implants

Description		Item No.
Straight Osseotite Tapered	Osteotome Kit	NTOST0
Angled Osseotite Tapered	Osteotome Kit	NTOST0A
Straight Osseotite Tapered, 3.25 mmD	Osteotome	NTOST3
Straight Osseotite Tapered, 4 mmD	Osteotome	NTOST4
Straight Osseotite Tapered, 5 mmD	Osteotome	NTOST5
Straight Osseotite Tapered, 6 mmD	Osteotome	NTOST6
Angled Osseotite Tapered, 3.25 mmD	Osteotome	NTOST3A
Angled Osseotite Tapered, 4 mmD	Osteotome	NTOST4A
Angled Osseotite Tapered, 5 mmD	Osteotome	NTOST5A
Angled Osseotite Tapered, 6 mmD	Osteotome	NTOST6A
Straight Osseotite Tapered	Osteotome Tray	NTOSTTRS
Angled Osseotite Tapered	Osteotome Tray	NTOSTTRA



Summers Osteotomes

Available for use with Parallel Walled Implants

Description	Item No.
Summers Osteotome Kit #1-4	OST00
Summers Osteotome Kit #1-5	OST10
Summers Osteotome Kit #1-5, FS	OST20
Summers Osteotome #1	OST01
Summers Osteotome #2	OST02
Summers Osteotome #3	OST03
Summers Osteotome #4	OST04
Summers Osteotome #5	OST05
Summers Osteotome for Future Site	OSTFS
Summers Osteotome System Tray	OSTTR



Sinus Elevators

Description	Item No.
Sinus Elevation Kit	SEKT1
Titanium Nitride Coated Bone Carrier	TIBC1
Small Membrane Elevator	ME100
Medium Membrane Elevator	ME200
Large Membrane Elevator	ME300
Large Titanium Plugger	TIPL1
Small Titanium Plugger	TIPS1
Sinus Elevation Tray	SEKTR



Trephine Burs

Description	Item No.
Trephine Bur, 2 mm Inside Diameter/3 mm Outside Diameter	TRE02
Trephine Bur, 4 mm Inside Diameter/5 mm Outside Diameter	TRE04
Trephine Bur, 5 mm Inside Diameter/6 mm Outside Diameter	TRE05
Trephine Bur, 6 mm Inside Diameter/7 mm Outside Diameter	TRE06
Trephine Bur, 8 mm Inside Diameter/9.3 mm Outside Diameter	TRE08



D = Diameter • P = Restorative Platform

Miscellaneous Instrumentation


Site Preparation Technologies

Description	Item No.
High Torque Indicating Ratchet Wrench	H-TIRW*
Open End Wrench For use with External Connection Implants.	CW100
Mallet Stainless Steel	MALL1
Implant Depth Gauge	DP020
Ratchet Extension, 6 mmL	RE100
Ratchet Extension, 15 mmL	RE200
Titanium Elevator	TE003
L-TIRW Standard ISO 1797 Adapter	C9980*
Tissue Measuring Post	TMP80



* H-TIRW, L-TIRW and associated adapters are manufactured by Elos Medtech AB and distributed by Zimmer Biomet Dental.

Description		Item No.
ACT Drill Extension		ACTDE
Gelb Radiographic Depth Gauge Kit - 2 mmD		XDG00
includes:	2 mmD x 13 mmL	XDG13
	2 mmD x 20 mmL	XDG20
Gelb Radiographic Depth Gauge Kit - 2.3 mmD		XDG01
includes:	2.3 mmD x 13 mmL	XDG2313
	2.3 mmD x 20 mmL	XDG2320
Handpiece Connector		MDR10
Tissue Punch, 4.1 mm		TP001
Tissue Punch, 5 mm		TP005
Tissue Punch, 6 mm		TP006

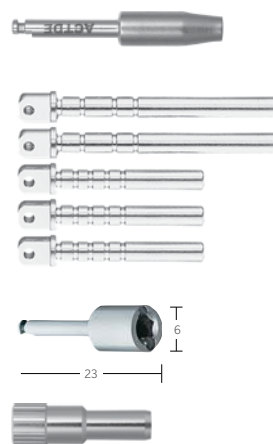

BellaTek Encode Impression System

(Available for Certain and External Hex Connections)

The BellaTek Encode Impression System eliminates the need for an implant-level impression while delivering a patient-specific restoration that has the appropriate margin height and natural emergence contours for the patient. This accuracy is achieved from an impression of the BellaTek Encode Healing Abutment. Codes embedded on the occlusal surface of the BellaTek Encode Healing Abutment communicate the collar height, implant hex-orientation, platform diameter and interface of the implant. Because the tissue is healed at the time of impression, the margin is designed to have the appropriate placement and contour. The result is a patient-specific, anatomically designed, final BellaTek Abutment.

Efficient Workflow For The Entire Team

The process is simplified with the BellaTek Encode Healing Abutment!

Surgeon

- Efficient, streamlined interoffice processes simplify treatment for the referring dentist.
- Cutting-edge technologies create an improved and more simple treatment process, differentiating the practice to referring dentists and more importantly, to patients.
- The BellaTek Encode Impression System makes it easier for your referral base and may increase treatment acceptance.

Laboratory

- Potential new customers may lead to increased crown and bridge business.
- There is no need to create a cast, which results in less steps in the treatment process, reducing overhead.
- This unique branding opportunity may grow the volume of your business.

The Result: A Highly Aesthetic BellaTek Definitive Abutment

Restorative Clinician

- Comfort: There is no need to use impression copings, resulting in a less invasive impression procedure for more comfort.
- Fewer Visits: The intraoral scan can be taken by the specialist at the surgical release visit, eliminating a restorative appointment and resulting in less visits to the dentist's office.
- Aesthetic Outcomes: Abutments designed specifically for the patient for better aesthetic outcomes.



BellaTek Encode Healing Abutment




BellaTek Abutments

Titanium
Nitrate
Coating


BellaTek Encode

Restorative Platform	Emergence Profile	Collar Height			
		3 mmH	4 mmH	6 mmH	8 mmH
3.4 mmD	3.8 mmP	EHA343	EHA344	EHA346	EHA348
	5 mmP	EHA353	EHA354	EHA356	EHA358
4.1 mmD	4.1 mmP	EHA443	EHA444	EHA446	EHA448
	5 mmP	EHA453	EHA454	EHA456	EHA458
	6 mmP	EHA463	EHA464	EHA556	EHA468
5 mmD	5.6 mmP	EHA553	EHA554	EHA556	EHA558
	6 mmP	EHA563	EHA564	EHA566	EHA568
6 mmD	6.8 mmP	EHA663	EHA664	EHA666	EHA668




EP One-Piece

Restorative Platform	Emergence Profile	Collar Height				
		2 mmH	3 mmH	4 mmH	6 mmH	8 mmH
3.4 mmD	3.8 mmP	MHA32	MHA33	MHA34	MHA36	—
4.1 mmD	4.1 mmP	THA42	THA43	THA44	THA46	THA48
	5 mmP	THA52	THA53	THA54	THA56	THA58
	6 mmP	—	THA63	THA64	THA66	THA68
5 mmD	5.6 mmP	WTH52	WTH53	WTH54	WTH56	WTH58
	6 mmP	WTH562	WTH563	WTH564	WTH566	WTH568
6 mmD	6.8 mmP	WTH62	WTH63	WTH64	WTH66	WTH68



Occlusal markings provide scanner information for abutment design.

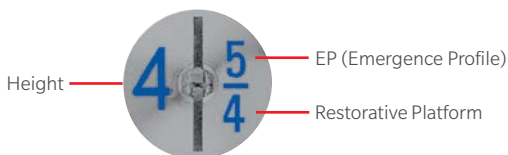

Temporary Healing Retention Cylinder Retains denture with soft tissue liner.	
THRC4	THRC6
4.1 mmD x 4.0 mmH	4.1 mmD x 6.0 mmH

PreFormance Posts*

Material: PEEK: Titanium Alloy Connection

Indications:

- Single- and multiple-unit cement-retained provisional restorations
- Minimum interarch space of 7 mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days
- Immediate nonocclusal loading of single-unit provisional restorations
- Multiple-unit restorations will require an evaluation of occlusal forces in lateral and protrusive excursions and masticatory forces to minimize the load on the provisional restorations
- Guided soft-tissue healing of single and multiple-unit restorations of integrated implants



Restorative Platform	Emergence Profile	Collar Height			
		4 mmH		6 mmH	
		Straight	15° Pre-Angled	Straight	15° Pre-Angled
3.4 mmD	3.8 mmP	MPPFP34	MPAPF34	MPPFP36	MPAPF36
4.1 mmD	5 mmP	PFP454	PAPF454	PFP456	PAPF456
5 mmD	5 mmP	WPPFP554	PAPF554	WPPFP556	PAPF556
6 mmD	6 mmP	WPPFP664	PAPF664	WPPFP666	PAPF666

Temporary Cylinders


Indications:

- Single- and multiple-unit screw-retained provisional restorations
- Minimum interarch space of 6 mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days for the PreFormance Temporary Cylinders
- Immediate nonocclusal loading of single-unit provisional restorations
- Multiple-unit restorations will require an evaluation of prosthesis support to minimize the load on the provisional abutments
- Occlusal loading of single- and multiple-unit restorations of integrated implants for guided tissue healing

PreFormance Temporary Cylinders*

Material: PEEK - Titanium Alloy Connection

Restorative Platform	Description	
	Hexed	Non-Hexed
3.4 mmD	MPFTC34	MPFTC32
4.1 mmD	PFTC41	PFTC42
5 mmD	WPFTC51	WPFTC52
6 mmD	WPFTC61	WPFTC62



Titanium Temporary Cylinders**

Material: Titanium Alloy Connection

Restorative Platform	Description	
	Hexed	Non-Hexed
3.4 mmD	MMTCS1	MMTCS2***
4.1 mmD	ITCS41	ITCS42
5 mmD	WTCS51	WTCS52
6 mmD	WTCS61	WTCS62



*All PreFormance Posts include the corresponding Titanium Hexed Screw (UNIHT).

**Titanium Temporary Cylinders are packaged with a Titanium Screw (IUNIHT) unless indicated otherwise.

***Screw not included.

D = Diameter • P = Emergence Profile • H = Collar Height


GingiHue Posts

Material:

- Commercially Pure Titanium (Straight Post)
- Titanium Alloy (Pre-Angled Post)

Indications:

- Single- and multiple-unit porcelain fused-to-metal restorations
- Areas of thin tissue where gingival discoloration is possible
- Preparable to follow gingival contours
- Conventional crown and bridge procedures
- Maximum angulation correction of 15°
- Minimum interarch space of 7 mm




Restorative Platform	Emergence Profile	Collar Height			
		2 mmH		4 mmH	
		Straight	15° Pre-Angled	Straight	15° Pre-Angled
3.4 mmD	3.8 mmP	MAP32G	MPAP32G	MAP34G	MPAP34G
	5 mmP	MAP352G	MPAP352G	MAP354G	MPAP354G
4.1 mmD	5 mmP	APP452G	PAP452G	APP454G	PAP454G
	6 mmP	APP462G	PAP462G	APP464G	PAP464G
5 mmD	5 mmP	WPP552G	PAP552G	WPP554G	PAP554G
	6 mmP	WPP562G	PAP562G	WPP564G	PAP564G
6 mmD	6 mmP	WPP662G	PAP662G	WPP664G	PAP664G

UCLA Abutments

Material: Machined Gold Alloy Cylinder With Plastic Unitube

Indications:

- Single- and multi-unit restorations
- Cement- and Screw-retained
- Laboratory fabricated custom abutments
- Minimum interarch space of 6 mm (4 mm - non-hexed)
- For aesthetic restorations when tissue is limited
- Maximum angulation correction of 30°



Description	3.4 mmD	4.1 mmD	5 mmD	6 mmD
Gold Standard ZR (Hexed) Abutment Cylinder	—	SGUCA1C	SWGUA51C	SWGUA61C
Gold (Hexed) Abutment Cylinder	MUCG1C	GUCA1C	WGA51C	WGA61C
Gold (Non-Hexed) Abutment Cylinder	MUCG2C	GUCA2C	WGA52C	WGA62C
Titanium Non-Hexed Abutment Cylinder	—	TUCA2C	—	—
Castable (Hexed) Abutment Cylinder	MUCC1C*	UNAB1C*	WPC51C*	WPC61C*
Castable (Hexed) Abutment Cylinder- 25Pk	—	UNA125*	—	—
Castable (Non-Hexed) Abutment Cylinder	MUCC2C*	UNAB2C*	WPC52C*	WPC62C*
Castable (Non-Hexed) Abutment Cylinder- 25Pk	—	UNA225*	—	—

* Not available in the US.

D = Diameter • P = Emergence Profile • H = Collar Height

Definitive Restorations

Restorative Components

GingiHue Post And UCLA Abutment Components

Pick-Up Impression Coping

Restorative Platform	Emergence Profile	Item No.
3.4 mm	3.8 mm	MIC33
4.1 mm	5 mm	IIC12
	6 mm	IIC60
	7.5 mm	IIC75
5 mm	5 mm	WIP55
	6 mm	WIP56
	7.5 mm	WIP57
6 mm	6 mm	WIP66
	7.5	WIP67



Twist Lock™ Impression Coping

Restorative Platform	Emergence Profile	Item No.
4.1 mm	5 mm	IIC45
	6 mm	IIC46
	7.5 mm	IIC47
5 mm	5 mm	WIT55
	6 mm	WIT56
	7.5 mm	WIT57
6 mm	6 mm	WIT66
	7.5 mm	WIT67







Laboratory Analog

Restorative Platform	Item No.
3.4 mmD	MMILA
4.1 mmD	ILA20
5 mmD	ILAW5
6 mmD	ILAW6






Additional Components

Description	3.4 mmD	4.1 mmD	5 mmD	6 mmD
Abutment Screw  	—	UNISG [*] , UNIHG 		
Sqaure Try-In Screw (5-pack)	MUNITS	UNITS		
Laboratory Abutment Holder 	LTAH5	LTAH7		

^{*}Recommended

Gold Alloy Cylinder Formulation	
Melting Range	1400–1490°C (2550–2710°F)
Solidus	1400°C
Liquidus	1490°C
CTE	12.2 x 10 ⁻⁶ °K at 500°C

Gold Alloy Cylinder Melting Temperatures		
	Fahrenheit	Celsius
Melting Range	2552-2732°F	1400-1500°C
Solidus	2552-2579°F	1400-1415°C
Liquidus	2714-2732°F	1490-1500°C
CTE	12.2 x 10 ⁻⁶ °K at 932°F	12.2 x 10 ⁻⁶ °K at 500°C

-  Requires the use of Hex Driver [PHD02N](#), [PHD03N](#) or Driver Tip [RASH3N](#), [RASH8N](#)
-  Requires the use of Impression Coping Driver [ICD00](#)
-  Requires the use of Square Driver [PSQD0N](#), [PSQD1N](#) or Driver Tip [RASQ3N](#), [RASQ8N](#)

Low Profile Abutments

Material: Titanium Alloy







Indications:

- Single- and multiple-unit screw-retained restorations
- Minimum interarch space of 7.5 mm
- Minimum tissue height of 1 mm
- Angle correction up to 30°
- Restorative platform 4.8 mm




Restorative Platform	Collar Height	Straight (Non-Hexed)	Straight (Hexed)	17° Pre-Angled (Hexed)	30° Pre-Angled (Hexed)
3.4 mmD	1 mm	LPC341U	LPC341	–	–
	2 mm	LPC342U	LPC342	LPAC3217	–
	3 mm	LPC343U	LPC343	–	LPAC3330
	4 mm	LPC344U	LPC344	LPAC3417	–
	5 mm	–	–	–	LPAC3530
4.1 mmD	1 mm	LPC441U	LPC441	–	–
	2 mm	LPC442U	LPC442	LPAC4217	–
	3 mm	LPC443U	LPC443	–	LPAC4330
	4 mm	LPC444U	LPC444	LPAC4417	–
	5 mm	–	–	–	LPAC4530
5 mmD	1 mm	LPC541U	LPC541	–	–
	2 mm	LPC542U	LPC542	LPAC5217	–
	3 mm	LPC543U	LPC543	–	LPAC5330
	4 mm	LPC544U	LPC544	LPAC5417	–
	5 mm	–	–	–	LPAC5530

Low Profile Abutment Components

Description	4.8 mm Restorative Platform	Description	4.8 mm Restorative Platform
Pick-Up Impression Coping (hexed) 	LPCPIC1	Gold Cylinder (hexed)	LPCGC1
Pick-Up Impression Coping (non-hexed) 	LPCPIC2	Gold Cylinder (non-hexed)	LPCGC2
Twist Lock Impression Coping (hexed) 	LPCTIC1	Castable Cylinder (hexed)	LPCCC1
Twist Lock Impression Coping (non-hexed) 	LPCTIC2	Castable Cylinder (non-hexed)	LPCCC2
QuickBridge® Impression Coping	LPCRIC	Laser Welded Cylinder 	LPCTUCA
Laboratory Analog	LPCLA	Waxing Screw	LPCWS
Temporary Cylinder (hexed)	LPCTC1	Retaining Screw	LPCGSH, LPCTSH
Temporary Cylinder (non-hexed)	LPCTC2	Lapping Tool	LPCAMI
Healing Cap 	LPCHC	Polishing Protector	LPCPP
PreFormance Temp. Cylinder (hexed)	LPCPTC1	Abutment Compatibility	
PreFormance Temp. Cylinder (non-hexed)	LPCPTC2	Component	Hexed Abutment
QuickBridge	LPCQB	Hexed	No
QuickBridge Replacement Cap	LPCQBCAP	Non-Hexed	Yes
Distal Extension	LPCDE		

 = Requires the use of Hex Driver [PHD02N](#), [PHD03N](#) or Driver Tip [RASH3N](#), [RASH8N](#)

 = Requires the use of Impression Coping Driver [ICD00](#)

D = Diameter • P = Emergence Profile • H = Collar Height

Overdenture Restorations

Restorative Components

LOCATOR R-Tx Abutments

Material:

Abutment: Titanium Alloy With DuraTec® Titanium Carbon Nitride Coating

Housing: Titanium Alloy with pink anodization.

Inserts: Nylon

Indications:

- Tissue supported removable overdentures on 2-4 implants
- Partially edentulous overdentures with one or more implants
- Limited interarch distance
- Angle correction with up to 60° between divergent implants

Collar Height	Restorative Platform	
	3.4 mmP	4.1 mmP
1 mmH	30305-01	30306-01
2 mmH	30305-02	30306-02
3 mmH	30305-03	30306-03
4 mmH	30305-04	30306-04
5 mmH	30305-05	30306-05
6 mmH	30305-06	30306-06



LOCATOR R-Tx Abutment Components

Description	Item No.
Zero Retention Insert - Grey, 4-pack	30001-01*
Low Retention Insert - Blue, 4-pack	30002-01*
Medium Retention Insert - Pink, 4-pack	30003-01*
High Retention Insert - Clear, 4-pack	30004-01*
Extra High Retention Insert - Green, 4-pack	30005-01
Processing Insert, 4-pack	30012-01
Denture Attachment Processing Assembly, 4-pack	30013-01*
3.35 mm Abutment Analog, 4-pack	30014-01
4 mm Abutment Analog, 4-pack	30015-01
5 mm Abutment Analog, 4-pack	30016-01
Impression Coping, 4-pack	30017-01
Processing Spacer, 4-pack	30018-01
Block-Out Spacer, 20-pack	08514*



* Included with each LOCATOR R-Tx Abutment.

LOCATOR R-Tx Abutment Tools

Description	Item No.
Retention Insertion Tool	30021-01
Hexed Driver Short, 7 mmL	PHD02N
Hexed Driver Long, 24 mmL	PHD03N
Hexed Driver Tip Short, 24 mmL	RASH3N
Hexed Driver Tip Long, 30 mmL	RASH8N



LOCATOR R-Tx May Not Be Available In All Markets.

LOCATOR Abutments

Material:

Abutment: Titanium Alloy With Gold-Colored Titanium Nitride Coating


Housing: Titanium Alloy

Inserts: Nylon

Indications:

- Tissue supported removable overdentures on 2-4 implants
- Partially edentulous overdentures with 1 or more implants
- Limited interarch distance
- Angle correction with up to 40° between divergent implants

Collar Height	Restorative Platform	
	3.4 mmP	4.1 mmP
1 mmH	MLOA001	LOA001
2 mmH	MLOA002	LOA002
3 mmH	MLOA003	LOA003
4 mmH	MLOA004	LOA004
5 mmH	MLOA005	LOA005
6 mmH	MLOA006	LOA006



LOCATOR Abutment Components

Description	Item No.
Standard Replacement Insert - White, 4-pack	LARMS*
Extra Light Retention Insert - Blue, 4-pack	LAELM*
Light Retention Replacement Insert - Pink, 4-pack	LLRMS*
Extended Range Inserts - Green, 4-pack	LAERM
Extra Light Retention Extended Range Insert - Red, 4-pack	LELARM
Replacement Housing	LOAH*
Replacement Housing Kit	LORHK
Block-Out Spacer, 20-pack	08514*
Impression Coping (one time use)	LAIC1
Laboratory Analog	LALA1



* Included with each LOCATOR Abutment.

LOCATOR Abutment Tools

Description	Item No.
Core Tool/Abutment Driver, 3-in-1 instrument	LCTDR1
Male Extraction Tool	LOA8397**
Abutment Driver Tip Short, 24 mmL	LOADT4
Abutment Driver Tip Large, 30 mmL	LOADT9
0.05 in/1.25 mm Hex Driver Tip 24 mmL - used with LCTDR1	RASH4
0.05 in/1.25 mm Hex Driver Tip 30 mmL - used with LCTDR1	RASH9

**Part of the Core Tool/Abutment Driver LCTDR1.

Restorative Components

Abutment Screws



	Gold-Tite® Square	Gold-Tite Hexed	Titanium Hexed
Screws	UNISG	UNIHG	UNIHT
Drivers	PSQD0N, PSQD1N	PHD02N, PHD03N	PHD02N, PHD03N
Driver Tips	RASQ3N, RASQ8N	RASH3N, RASH8N	RASH3N, RASH8N
Torque	32–35 Ncm	20 Ncm	20 Ncm
For Use With:	UCLA Abutment, GingiHue Post, GingiHue Post 15°, Temporary Cylinder		

Retaining Screws



	Low Profile Abutment Gold-Tite Screw	Low Profile Abutment Titanium Screw	Gold-Tite Screw	Titanium Hexed Screw
Screws	LPCGSH	LPCTSH	GSH20, GSH30, GSH70	TSH30
Drivers	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N
Driver Tips	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N
Torque	10 Ncm	10 Ncm	10 Ncm	10 Ncm
For Use With:	Low Profile Abutment	Low Profile Abutment	GSH20 - Standard Abutment 6.0 mmD X 2.0 mmH Conical Abutment 6.0 mmD X 1.0 mmH GSH30 - Standard, Conical and IOL® Abutments GSH70 - Standard, Conical and IOL Abutments	Standard, Conical and IOL Abutments

Waxing Screws And Try-In Screws



	Abutment Waxing Screw/ Guide Pin	Laboratory Waxing Screw	Square Try-In Screw (5-pack)
Screws	WSK10, WSK15	WSK30, WSU30	UNITS, MUNITS
Drivers	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N
Driver Tips	RASH3N, RASH8N	RASH3N, RASH8N	RASH3N, RASH8N
For Use With:	Standard and Conical Abutments	Implant Level Laboratory Procedures	UCLA Abutment, GingiHue Post, GingiHue Post 15°

Restorative Components

BellaTek Bars and Frameworks are created with the technology to achieve a truly passive fit. This technology does not require any wax or resin design from the technician. Because these are milled from one solid piece of lightweight titanium, the potential for weakness caused by soldering or laser welded joints is eliminated. You receive a completed superstructure ready for prosthesis processing. No polishing or retention creation necessary. Zimmer Biomet Dental can even tap holes for attachments. Copymilled Bars are also available.

Hybrid Bar Design #1



- Fixed prosthesis
- Metal lingual
- Low buccal finish line
- Titanium tissue surface




Hybrid Bar Design #2



- Fixed prosthesis
- Metal lingual
- Low buccal finish line
- Titanium tissue surface



Wraparound Bar

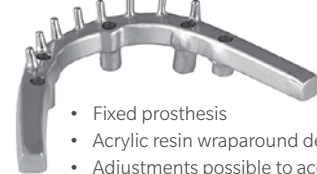

- Fixed prosthesis
- Acrylic resin wraparound design
- Adjustments possible to accommodate for changing tissue contours
- Easy to repair and modify the acrylic resin portion of the prosthesis



Freeform Bar



- Fixed prosthesis
- Acrylic resin wraparound design



DOLDER® Egg Shape Bar



- Removable overdenture design
- Anterior clips allow for anterior/posterior rotation of the overdenture
- Provides lateral stability to the overdenture



DOLDER U Shape Bar



- Removable overdenture design
- Anterior clips allow for anterior/posterior rotation of the overdenture
- Provides lateral stability to the overdenture



Hader Bar



- Removable overdenture design with clips that engage undercuts
- Provides lateral stability to the overdenture
- 4 mm between implants is needed for clips



Primary Bar



- Most secure removable overdenture design
- May be used with attachments or secondary casting
- Bar can be designed with a 2° – 6° taper




Combination Primary Bar With Hader Or DOLDER Designs



- Combines a milled bar with Hader or DOLDER Designs
- Provides excellent lateral stability to the overdenture
- Bar can be designed with a 2° – 6° taper



Design Features

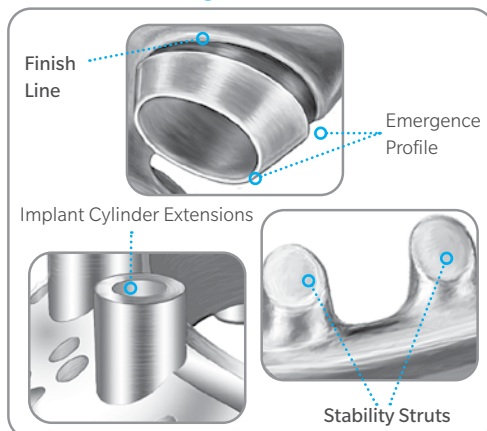

Copymilled Cobalt Chrome Framework*



- Fixed screw-retained prosthesis, allowing veneering of user friendly CoCr porcelains with CTE $14.1 \times 10^{-6} K^{-1}$
- High biocompatible Cobalt Chrome Alloy, certified for orthopedic surgical implants

Copymilled Titanium Framework



- Ideal for fixed screw-retained prosthesis. Scanned from a lab designed resin pattern
- Available in Titanium Alloy for acrylic Finishing or Commercially Pure titanium for Titanium porcelain veneer

Ask for these design features on the BellaTek Bars And Frameworks Work Order Form (ZB0230).

*Not available in the U.S.

Restorative Components

NCATD0

Contra Angle Torque Driver Kit*



NPSDK0

Prosthetic Driver Kit*



L-TIRWK

Low Torque Indicating Ratchet Wrench Kit**



Description	Item No.	Contra Angle Torque Kit			Prosthetic Driver Kit		Low Torque Indicating Kit	
		NCATD0	NPSDK0	L-TIRWK	NCATD0	NPSDK0	L-TIRWK	L-TIRWK
Narrow Posterior Hex Driver, 17 mmL	PHD02N	•	•					
Narrow Posterior Square Driver, 17 mmL	PSQD0N	•	•					
Contra Angle Torque Driver Body	HTD-C	•	•					
Narrow Right Angle Hex Driver Tip, 24 mmL	RASH3N	•	•	•				
Narrow Right Angle Hex Driver Tip, 30 mmL	RASH8N	•	•					
Right Angle Abutment Driver Tip - Steel	RASA3	•	•					
Narrow Right Angle Square Driver Tip, 24 mmL	RASQ3N	•	•	•				
Narrow Right Angle Square Driver Tip, 30 mmL	RASQ8N	•	•					
Contra Angle Torque Controller, 10 Ncm*	TD-10		•					
Contra Angle Torque Controller, 20 Ncm*	TD-20	•	•					
Contra Angle Torque Controller, 35 Ncm*	TD-35	•	•					
Contra Pre-action Handle	CATDH	•	•					
Prosthetic System Driver Tray	PSDT1	•	•					
Narrow Impression Coping Driver	ICD00		•					
Posterior Abutment Driver, 17 mmL	PAD00		•					
Standard Abutment Driver, 24 mmL	PAD24		•					
Posterior Slotted Screw Driver, 17 mmL	PSD00		•					
Standard Slotted Screw Driver, 24 mmL	PSD01		•					
Narrow Standard Slotted Square Driver, 24 mmL	PSQD1N		•					
Narrow Standard Hex Driver, 24 mmL	PHD03N		•					
Right Angle Slotted Driver Tip, 30 mmL	RASD1		•					
Low Torque Indicating Ratchet Wrench	L-TIRW**						•	
Restorative Torque Tray	RTI2035TR						•	

* NCATD0 and NPSDK0 are manufactured by NSK America Corp/NSK dental LLC and distributed by Zimmer Biomet Dental.

**L-TIRW, H-TIRW and associated adapters are manufactured by Elos Medtech AB and distributed by Zimmer Biomet Dental.

The cordless Prosthodontic Screwdriver has torque control, which enables precise tightening of retaining screws. This cordless screwdriver reduces the need for traditional mechanical rotary ratchet wrench systems.

Features Include:

- Torque control of 8-40 Ncm in 1 Ncm steps for precise tightening of retaining screws
- An automatic stop when the preset torque is reached
- Cordless operation with constant drive speed
- A small contra-angle head for better visibility of the treatment site
- A contra-angle that can be rotated 360°
- A clockwise and counter clockwise operation
- A sterilizable contra-angle

Prosthodontic Screwdriver IA-400

Includes:

- A handpiece drive IA-40H with keypad and rechargeable Li-Ion battery (not sterilizable)
- A contra-angle IA-80 with a hexagon chucking system
- A charging station with country specific cables available



Description	Item No.
IA-400 Prosthodontic Screw Driver	16934000
IA-400 Charging Station	05338301
IA-80 Contra-Angle Hand Piece, 80:1	16338001
IA-40H Handpiece Drive	16834000
Operation Lever	05937000
Power Cord US, CAN, J	05456100
Power Cord UK, IRL	05457700
Power Cord EU	05464400
Power Cord AUS, NZ	05467600
Rechargeable Battery, Li-Ion	05451300

Restorative Components




Length	Small Hex		Large Hex		Square	
	Driver	Tip	Driver	Tip	Driver	Tip
17 mm	PHD00N	—	PHD02N	—	PSQD0N	—
24 mm	PHD01N	RASH2N	PHD03N	RASH3N	PSQD1N	RASQ3N
30 mm	—	RASH7N	—	RASH8N	—	RASQ8N
For Use With:	External Hex Cover Screws		Healing Abutments, Abutment Screws, Certain Cover Screws and Retaining Screws		Square Gold-Tite® Abutment Screws and Square Try-in Screws	



Length	Abutment		LOCATOR®	Impression Coping	.050" Hex
	Driver	Tip	Driver	Driver	Tip Only
17 mm	PAD00	—	—	ICD00	—
24 mm	PAD24	RASA3	LOADT4	—	RASH4
30 mm	—	—	LOADT9	—	RASH9
For Use With:	Low Profile Abutments		LOCATOR Abutments	Twist Lock™ Transfer LOCATOR Abutments with Impression Copings	LOCATOR abutments with LOCATOR Core Tools

Restorative Components

Description		Item No.
Reamer and Handle		IRH600
Low Torque Indicating Ratchet Wrench		L-TIRW*
Low Torque Indicating Ratchet Wrench Kit		L-TIRWK
Polishing Protector	3.4 mmP	PPMM1
	4.1 mmP	PPIA3
	5 mmP	PPIA5
	6 mmP	PPIA6
Standard ISO 1797 Adapter		C9980*
Short ISO 1797 Adapter		C9981*
Prosthetic Angle Guide Kit, 15°, 25°, 35°		AG900
Tissue Measuring Post		TMP80

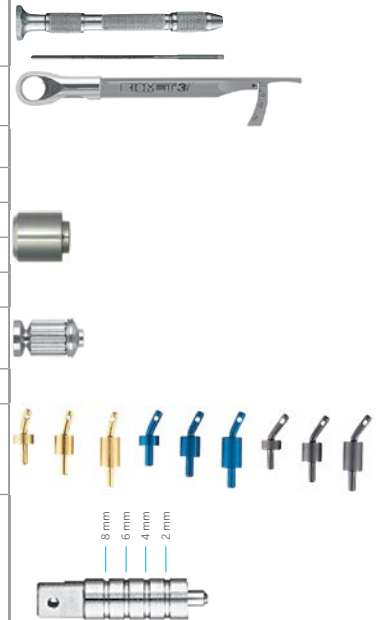

**L-TIRW, H-TIRW and associated adapters are manufactured by Elos Medtech AB and distributed by Zimmer Biomet Dental.

For comprehensive information, please see the Regenerative Product Brochure or visit www.zimmerbiometdental.com.







Contact us at 1-800-342-5454 or visit
zimmerbiometdental.com

Zimmer Biomet Dental
Global Headquarters
4555 Riverside Drive
Palm Beach Gardens, FL 33410
Tel: +1-561-776-6700
Fax: +1-561-776-1272

Unless otherwise indicated, as referenced herein, all trademarks are the property of Zimmer Biomet; and all products are manufactured by one or more of the dental subsidiaries of Zimmer Biomet Holdings, Inc. and marketed and distributed by Zimmer Biomet Dental and its authorized marketing partners. LOCATOR, LOCATOR R-Tx, R-Tx, Color and Shape of Retention Inserts, and DuraTec are registered trademarks of ZEST IP Holdings, LLC. LOCATOR Attachments are manufactured by ZEST Anchors, LLC. Implantmed is manufactured by W&H Dentalwerk Bürmoos GmbH. Implantmed and W&H are registered trademarks of W&H Dentalwerk Bürmoos GmbH. Dolder is a registered trademark of Dr. Charlotte Fleischer-Dolder and Dr. Fritz Dolder. For additional product information, please refer to the individual product labeling or instructions for use. Product clearance and availability may be limited to certain countries/regions. This material is intended for clinicians only and does not comprise medical advice or recommendations. Distribution to any other recipient is prohibited. This material may not be copied or reprinted without the express written consent of Zimmer Biomet Dental. ZBINST1262 REV D 03/21 ©2021 Zimmer Biomet. All rights reserved.

